

Guardian: Foot Plate and Hand Cylinder Use



A very prominent MD, experienced in energetic medicine, recommends using the Foot Plate (FP) and Hand Cylinders (HC) with the Guardian to gather vibrational information from the body.

The feet and hands possess many acupuncture points. Thus, by using the FP and HC, you are able to access and imprint the information coming from these points.

The **Transfer Box** allows you to use the FP and HC at the same time when making an imprint or when putting the amplified signal back into the body. Because the Transfer Box is also designed to be used with our MicroGen frequency generator, it has both a positive (**Red**) plug and a negative (**Black**) plug. When used with the Guardian; however, you will only use one of the **Red** plugs.

Imprinting the Vials

1. Connect the Guardian to the Transfer Box by using the short **Red** cable. The **Black** plug (3.5 mono-plug) should be plugged into the Guardian's INPUT jack on the side of the Guardian. The other end has a **Red** plug which must be plugged into the one of the **Red** jacks on the side of the Transfer Box as pictured below.
2. Plug the split cords into the FP and HC
3. Plug the other end (3.5 mono-plug) of the split cords into the top of the Transfer Box as pictured below.
4. Place two vials with imprinting solution on the **OUTPUT** side (right side) of the Guardian. Press the CLEAR button to clear any extraneous signal.
5. With both feet on the FP and holding the HC, press the **Activate** button on the Guardian.
6. The Guardian will now be gathering information from your body and running the signal through it's circuitry and imprinting the amplified signal into the two vials on the **OUTPUT** side.

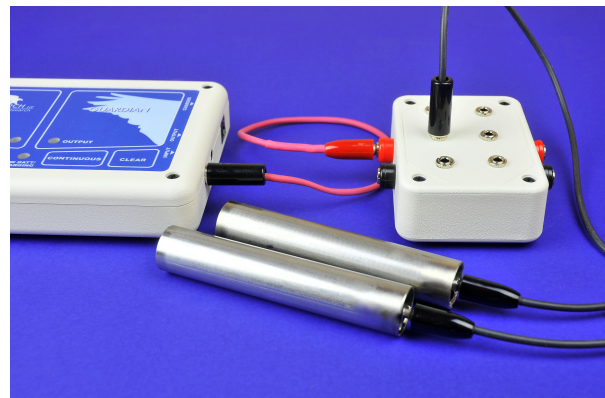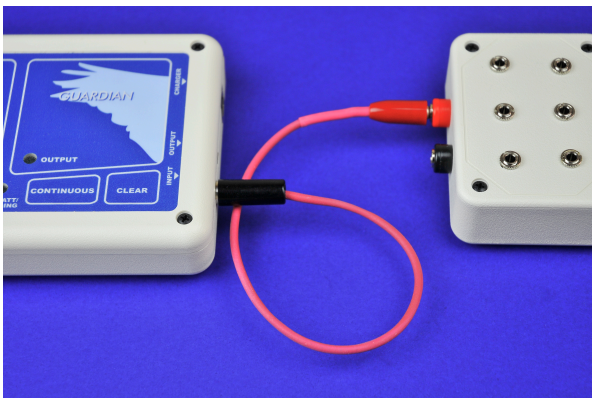

Guardian: Foot Plate and Hand Cylinder Use

Putting the Signal Back Into The Body

1. Once the vials have been imprinted, we recommend succussing the vials about 50 times.
2. Move one of the vials to the **INPUT** (left side) of the Guardian and set the other vial aside. (Your practitioner may have you wear this vial on your person. We call this the “Body Vial” and it radiates the imprinted signal continuously.)
3. Now, **unplug** the **Red** cable from the Guardian’s **INPUT** and plug it into the **OUTPUT** on the side of the Guardian.
4. With both feet on the FP and holding the HC, once again press the **Activate** button. This time the Guardian is picking up the amplified signal in the vial on the INPUT side and putting this amplified signal back into the body through the **OUTPUT** of the Guardian and through the foot plate and hand cylinders.
5. If you wish to input the signal for an extended period of time, you may press the **CONTINUOUS** button instead of the **ACTIVATE** button. Consult your practitioner for recommendations.

WARNING: The Transfer Box has a RIGHT side and a LEFT side. The **Red** and **Black** plugs on the right side only supply a signal to the three silver plugs on the top, right side. The **Red** and **Black** plugs on the LEFT side only supply a signal to the three silver plugs on the top LEFT side. This means that accessories **MUST** be plugged into one of the three plugs on the **same side** that the **Red** cable is plugged into.

